


Tensile test fixture to test bonding strength of dental prostheses according to DIN EN ISO22112 and DIN EN ISO20795-1

Item no.:	THS1447-S12 + TH227+BP25
Max. load:	2 kN
Coupling:	Af159 or Af20. Further couplings on request.
Material:	Steel, aluminium, plastic
Temperature range:	0 ... +70°C Further temperature ranges on request
Scope of supply:	1 fixture consisting of top and bottom grips

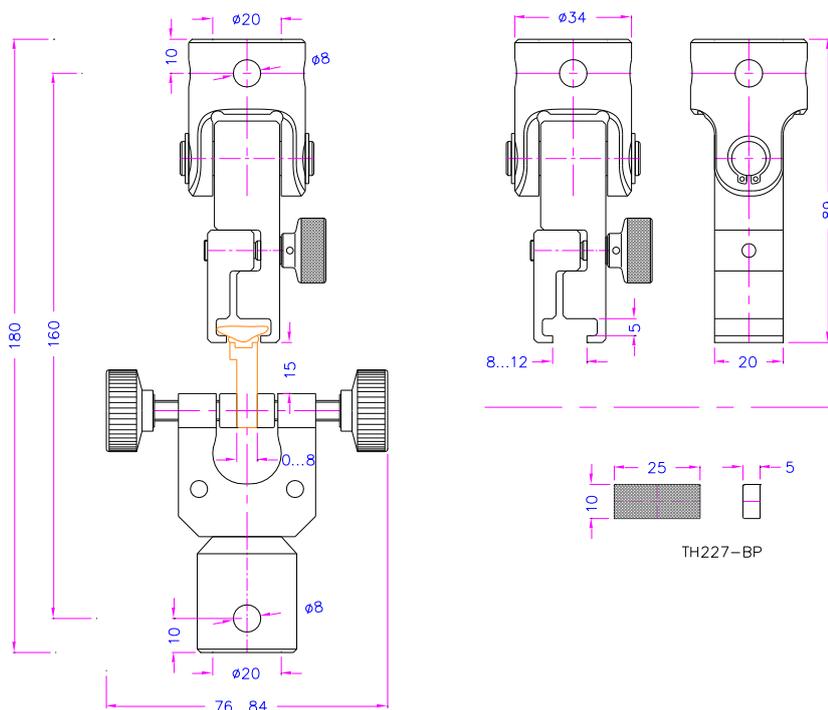

We recommend **TH227+BP25** as the bottom grip